

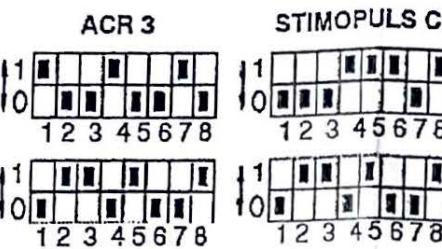


STIMOPULS C, MA, AUTOPULS C and ACR3

The electronic board is provided with the STIMOPULS C setup (view settings below). If you require another version, please refer to coding below :

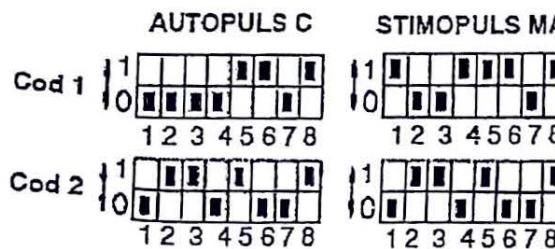

Factory setup

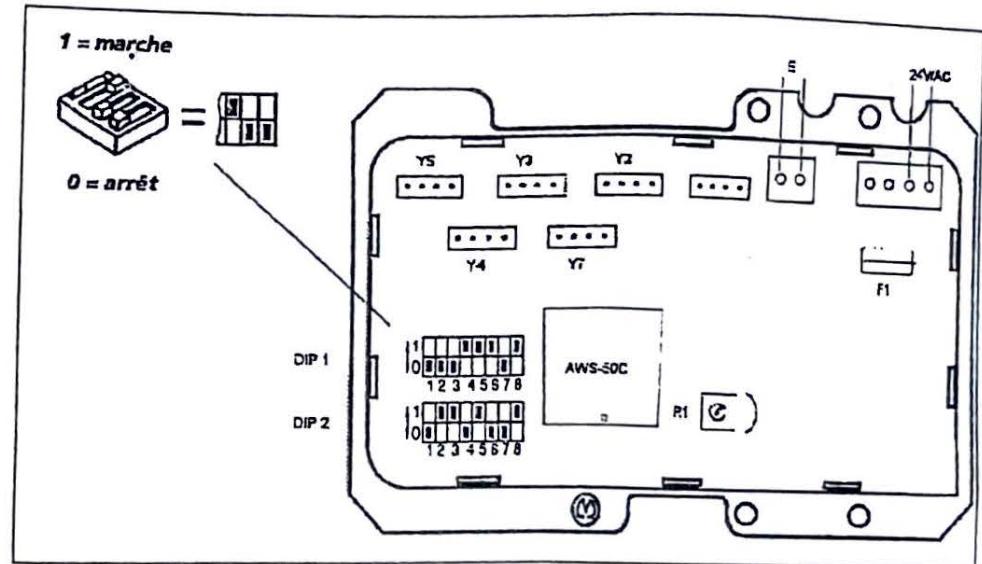

The electrode resistor is set at 460 Ohms (VISOFLOW milk flow monitor).

For more information, please refer to the GEA Westfalia documentation.